

Bio-Design and Manufacturing

FUNCTIONALLY GRADED ADDITIVE MANUFACTURING TO ACHIEVE FUNCTIONALITY SPECIFICATIONS OF OSTEOCHONDRAL SCAFFOLDS

--Manuscript Draft--

Manuscript Number:							
Full Title:	FUNCTIONALLY GRADED ADDITIVE MANUFACTURING TO ACHIEVE FUNCTIONALITY SPECIFICATIONS OF OSTEOCHONDRAL SCAFFOLDS						
Article Type:	Personal View						
Funding Information:	<table border="1" style="width: 100%;"> <tr> <td style="width: 60%;">H2020-MSCA-RISE (734156)</td> <td style="width: 40%;">Prof. Mario D. Monzón</td> </tr> </table>	H2020-MSCA-RISE (734156)	Prof. Mario D. Monzón				
H2020-MSCA-RISE (734156)	Prof. Mario D. Monzón						
Abstract:	Osteoarthritis (OA) is a degenerative joint disease, characterised by cartilage loss and changes in bone at the interface of a joint resulting in pain, stiffness and reduced mobility. OA is one of the most prevalent chronic conditions as identified in Bone and Joint Decade. According to the World Health Organisation 40% of people over the age of 70 have OA. The aim of this paper is to define the functionality and performance which would be required for intended clinical applications in the treatment of osteoarthritis. Also, to show that the capabilities of 3D bioprinting and functionally graded additive manufacturing scaffolds are suitable to meet most of these requirements.						
Corresponding Author:	Mario D. Monzón, PhD Universidad de las Palmas de Gran Canaria Las Palmas de Gran Canaria, Canarias SPAIN						
Corresponding Author Secondary Information:							
Corresponding Author's Institution:	Universidad de las Palmas de Gran Canaria						
Corresponding Author's Secondary Institution:							
First Author:	Mario D. Monzón, PhD						
First Author Secondary Information:							
Order of Authors:	<table border="1" style="width: 100%;"> <tr><td>Mario D. Monzón, PhD</td></tr> <tr><td>Chaozong Liu</td></tr> <tr><td>Sara Ajami</td></tr> <tr><td>Miguel Oliveira</td></tr> <tr><td>Ricardo Donate</td></tr> <tr><td>Viviana Ribeiro</td></tr> </table>	Mario D. Monzón, PhD	Chaozong Liu	Sara Ajami	Miguel Oliveira	Ricardo Donate	Viviana Ribeiro
Mario D. Monzón, PhD							
Chaozong Liu							
Sara Ajami							
Miguel Oliveira							
Ricardo Donate							
Viviana Ribeiro							
Order of Authors Secondary Information:							
Author Comments:	The article type is: SHORT PAPER						
Suggested Reviewers:	<table border="1" style="width: 100%;"> <tr> <td>Suny Martinez, Dr. AIJU technological center sunymartinez@aiju.info Expertise in additive manufacturing processes and polymers</td> </tr> <tr> <td>Eoin Cunningham, Dr. Queens university of Belfast e.cunningham@qub.ac.uk Expertise in byopolimers for medical applications</td> </tr> </table>	Suny Martinez, Dr. AIJU technological center sunymartinez@aiju.info Expertise in additive manufacturing processes and polymers	Eoin Cunningham, Dr. Queens university of Belfast e.cunningham@qub.ac.uk Expertise in byopolimers for medical applications				
Suny Martinez, Dr. AIJU technological center sunymartinez@aiju.info Expertise in additive manufacturing processes and polymers							
Eoin Cunningham, Dr. Queens university of Belfast e.cunningham@qub.ac.uk Expertise in byopolimers for medical applications							

[Click here to view linked References](#)

SHORT PAPER

FUNCTIONALLY GRADED ADDITIVE MANUFACTURING TO ACHIEVE FUNCTIONALITY SPECIFICATIONS OF OSTEOCHONDRAL SCAFFOLDS

Mario Monzón

Departamento de Ingeniería Mecánica, Universidad de Las Palmas de Gran Canaria, 35017 Las Palmas G.C., Spain, phone: +34928458617, e-mail: mario.monzon@ulpgc.es

Chaozong Liu

Division of Surgery & Interventional Science, University College London, Stanmore, London HA7 4LP, UK, phone: 020 8954 9427, e-mail: chaozong.liu@ucl.ac.uk

Sara Ajami

Division of Surgery & Interventional Science, University College London, Stanmore, London HA7 4LP, UK, phone: 020 8954 9427, e-mail: sara.ajami@ucl.ac.uk

Miguel Oliveira

3Bs Biomaterials, biodegradables and biomimetics, Universidade Do Minho, Parque de Ciência e Tecnologia Zona Industrial da Gandra, Barco GMR, 4805-17, Portugal, phone: 351253510900, e-mail: miguel.oliveira@dep.uminho.pt

Ricardo Donate

Integrated and advanced manufacturing processes research group, edificio de ingenierías, Universidad de Las Palmas de Gran Canaria, 35017 Las Palmas G.C., Spain, phone: +34928458603, e-mail: ricardo.donate@ulpgc.es

Viviana Ribeiro

3Bs Biomaterials, biodegradables and biomimetics, Universidade Do Minho, Parque de Ciência e Tecnologia Zona Industrial da Gandra, Barco GMR, 4805-17, Portugal, phone: 351253510900, e-mail: viviana.ribeiro@dep.uminho.pt

INTRODUCTION

Osteoarthritis (OA) is a degenerative joint disease, characterised by cartilage loss and changes in bone at the interface of a joint resulting in pain, stiffness and reduced mobility. OA is one of the most prevalent chronic conditions as identified in Bone and Joint Decade. According to the World Health Organisation 40% of people over the age of 70 have OA. This joint disease affects around 0.4 billion people with patients in Europe accounting for up to 30%. The figure is set to increase with the ageing problem.

Current non-surgical treatments for OA involve non-steroidal anti-inflammatory drug administration. Surgical treatments include osteotomy, abrasion arthroplasty, microfracture and autologous chondrocyte implantation (ACI). This is a two stage surgical procedure with the associate costs and infection being the main concern. For small osteochondral defects, microfracture (MF) marrow stimulation and for large cartilaginous defects the autologous chondrocyte implantation are considered as necessary treatments. However, MF produces fibrocartilage not native hyaline cartilage. While for defects that have progressed to a stage that affects the subchondral bone, other treatments are no longer effective and joint replacement operation is the only alternative.

1 The demand for innovative therapeutic alternatives for complete healing of OA is significant. The
2 treatment of cartilage and osteochondral (OC) defects remains a challenge since treatments so far
3 have failed to achieve complete restoration of the properties of joint cartilage. Many new
4 technologies, such as osteochondral tissue engineering, have been studied and applied to repair
5 osteochondral defects. Commercially available osteochondral scaffolds have been used in patients
6 with OC defects. However, no products have so far demonstrated to provide biomechanical
7 properties suitable to promote the durable regeneration of large OC defects [1]. The main issue
8 with these commercially available OC scaffolds is poor cartilage fill associated with fibrocartilage
9 formation.

10
11 The aim of this paper is to define the **functionality and performance** which would be required
12 for intended clinical applications in the treatment of osteoarthritis. Also, to show that the
13 capabilities of **3D bioprinting** and **functionally graded additive manufacturing scaffolds** are
14 suitable to meet most of these requirements.
15

16 17 18 **COMMERCIAL OSTEOCHONDRAL SCAFFOLDS AND CLINICAL PERFORMANCE** 19

20 Treatments using tissue engineering methods have been established and are promising for the
21 treatment of small osteochondral defects.
22

23 Biphase scaffolds have represented many relevant progresses for osteochondral reconstruction
24 in vivo or preclinical test. Multi-layered scaffolds, consisting of bone- and cartilage-like layers,
25 seem to be the most promising approach to achieve the regeneration of OC defects [2]. Moreover,
26 a few novel bilayer scaffolds have been approved for clinical implementation: MaioRegen® [3-
27 4] and TruFit™ Plug [5-6].
28
29

30 MaioRegen® is a bilayer scaffold mimicking the OC unit. The superficial layer is composed of
31 Col I and is similar to the cartilaginous tissue, while, the bottom layer consists mostly of
32 magnesium-enriched hydroxyapatite (Mg-HA), similar to the subchondral bone structure [7]. The
33 intermediate layer of collagen and Mg-HA replicates the tide-mark. TruFit™ plug is a bilayer
34 scaffold composed of PLGA fibre and calcium sulfate (CaSO₄).
35
36

37 MaioRegen® has been systematically studied in patients. The international knee documentation
38 committee (IKDC) reported that subjective score of the suffer knee was significantly improved.
39 Similar positive conclusion was confirmed by the visual analogue scale and Tegner scores at 24
40 months after implantation [8]. These results showed that this was a good strategy for OCD
41 treatment but abnormal magnetic resonance imaging findings were presented [9]. Another study
42 was carried out in 11 patients for the treatment of tibial plateau lesions. An acceptable clinical
43 behaviour was reported at 2 years follow-up [10]. Recently, Christensen et al. [11], investigated
44 the analogous results of bilayer MaioRegen® for osteochondral defect repair after 1–3 years
45 clinical and radiological observation. Incomplete cartilage repair and poor subchondral bone
46 repair was found at 1 and 2.5 years follow-up. Nevertheless, the clinical scores were significantly
47 improved.
48
49

50 Agili-C™ (CartiHeal, Israel) is another recently developed osteochondral scaffold consisting of
51 a natural crystalline aragonite, derived from corals, to which hyaluronic acid (HA) is added [12].
52 The natural aragonite, possess a nano-rough structure as well as interconnecting porosity that
53 allows to stimulate cell adhesion and proliferation as well as matrix production.
54
55

56 To summarize, for the success of osteochondral tissue engineering the primary requirements of
57 scaffolding materials include biocompatibility, biodegradability, mechanical stability, and pore
58 structure:
59
60
61
62
63
64
65

Biocompatible and degradable materials

It is well known that scaffolds must be fabricated from biocompatible materials which do not stimulate immune responses or foreign body reactions. In addition, the biodegradation of scaffolds during in vivo treatment should closely match tissue growth rates [13]. Facilitating regeneration of cartilage requires that the implanted scaffold remain stable for at least two-three weeks. Stability of the scaffold in this period allows sufficient time for the composition of support structures for subsequent regeneration of tissues.

Mechanical stability

Osteochondral interfacial tissue has different mechanical strengths depending on the property at each stratified layer. Mismatched viscoelastic properties of osteochondral tissue lead to stress disparities between cartilage tissues. Superficial cartilage can withstand a local compressive stress of 0.08– 2 MPa, tensile modulus of 5–25 MPa, and equilibrium shear modulus of 0.05–0.25 MPa [14]. These differences arise from the biological and chemical composition and thereby from mechanical strengths in each zone. In order to optimize resistance in osteochondral tissue, superficial collagen exists parallel to the shear direction, while collagen in the deep zone is perpendicular to the surface. Owing to this highly organized structure and its properties, artificial recreation of this tissue is still challenging. Intensive progress on remodelling cartilage has been made using transforming growth factor- β 1 (TGF- β 1) and mechanical stimulation to improve its tensile modulus up to more than 3.4 MPa [15].

Pore structure

The pore structures affect the cell responses and their further organization in the tissue, regulating cell invasion, vascularization, and tissue regeneration in most scaffolds. In several studies on the effects of pore size, scaffold structures composed of porosity higher than 50% and pores larger than 300 μ m is recommended to achieve direct osteogenesis with enhanced vascularization [16]. On the contrary, pores of 90–120 μ m have been suggested for favourable chondrogenesis, where MSCs proliferate and form cartilage tissue on the scaffold [17].

HOW ADDITIVE MANUFACTURING CAN COMPLY WITH REQUIREMENTS FOR THE CLINICAL PERFORMANCE OF OC SCAFFOLDS

The **Additive Manufacturing (AM)** technology is based on solid freeform manufacturing for the direct production of complex parts without resorting to specific moulds and tools [18]. According to ISO/ASTM 52900:2015 [19], AM is defined as “process of joining materials to make parts from 3D model data, usually layer upon layer, as opposed to subtractive manufacturing and formative manufacturing methodologies”. AM is a multidisciplinary field requiring close interaction between design, material, technology and information and communication technologies (ICT). At present, AM involves procedures for the addition of material layer by layer starting from 3D solid CAD. ISO/ASTM 52900:2015 has categorized AM processes into seven areas:

- 1. Binder jetting:** It uses liquid bonding agent to join powder materials.
- 2. Directed energy deposition:** Focused thermal energy is used to fuse materials by melting as they are being deposited.
- 3. Material extrusion:** The material is selectively dispensed through a nozzle.

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65

4. **Material jetting:** Droplets of build material are selectively deposited.

5. **Powder bed fusion:** Thermal energy selectively fuses regions of a powder bed.

6. **Sheet lamination:** Sheets of material are bonded.

7. **Vat photopolymerization:** A liquid photopolymer in a vat is selectively cured by light



Figure 1. Micro features by DLP part (total part size 7x7x0.5 mm). Pixelation structure due to resolution of DLP. Courtesy University of Las Palmas de Gran Canaria.

Some of these procedures are very suitable for **micro-manufacturing**, with high potential in tissue engineering due to the small size of features or texture. For example, in the group of Vat photopolymerization is well known the **Digital Light Processing (DLP)**, which is based on an array of micro-mirrors suitable to be oriented into two positions, moved by micro-actuators. The UV light is reflected by these micro-mirrors to the layer of liquid photopolymer, curing each layer like a unique mask [20]. The resolution of the cured mask is defined by the number of pixels. Figure 1 shows the level of detail for small features (diameter of pins 0.15 mm, side length of squares 0.09 mm, diameter of holes 0.1 mm). Also, the pixelation due to the resolution of the mask (in this example the size of each pixel is about 40 microns) can be observed. The availability of hydrogels based on photopolymers becomes this DLP system in a very promising technology for bioprinting at micro level, not so easy to achieve in extrusion based technologies such as the bioplotters, as described in the following paragraphs.

Among the previous methods, powder bed fusion is mainly used for titanium alloy scaffolds (SLM or EBM) [21]. However, the bioinert nature of this material inhibits osteointegration with the surrounding tissue. Several companies have developed bioprinters to take advantage of the capabilities of additive manufacturing to produce complex scaffolds. Several natural and synthetic polymers, bioactive inorganic materials, and their combinations have been employed for bone and cartilage tissue engineering and regeneration. Nevertheless, not all the biomaterials are suitable to be printed by these technologies. In particular for those **extrusion based bioplotters** the **extrudability of either biopolymers or bioinks** is the main factor to take into account from the point of view of the processability. Temperature and viscosity are key factors in order to achieve good quality of material as well as accuracy of the porous/lattice structure. Many natural biopolymers (chitosan, alginate, collagen) processed as hydrogels, have the advantage of less restrictive parameters of processing and no needs of toxic solvents. These can be either processed by the method of material extrusion (with chemical crosslinking) or Vat photopolymerization (crosslinking by UV light). Otherwise, material jetting requires very low viscosity of the biopolymer (below 10 cP) [22] limiting the availability of materials. Table 1 shows a summary of some commercial extrusion based bioplotters as well as available bioinks [23].

Table 1. Commercial bioplotters and biomaterials for 3D printing

Model, Company	Material
3D Bioplotter, Envisiontec	Ceramic/metal pastes (HA, TCP, Ti), thermoplastics (PCL, PLLA, PLGA), Hydrogels (Agar, Gelatin, Soy, Hyaluronic acid, Alginate, fibrin, chitosan, collagen), acrylates (UV curing)
BIO X., CELLINK	Alginate/nanocellulose, collagen, gelatin methacrylate, Pluronic F127 (polypropylene glycol/polyethylene glycol), TCP, PCL,
Biofactory, RegenHU	PEG, gelatin, hyaluronic acid-based, Calcium phosphate
Allevi 6, Allevi	PLGA, PCL, Pluronic 127, gelatin methacrylate, collagen, alginate, fibrin, Polyethylene glycol diacrylate

One relevant feature of a bioplotter is the option of depositing multi-materials by **multi print heads**. This option provides making multimaterial scaffolds combining, for example, hydrogels with biopolymers, following different strategies. For instance, Shim, et al. [24], combined synthetic materials such as PCL or PLGA with hyaluronic acid, gelatin or collagen based, by alternative extrusion of these materials in a multi print head extruder, observing a significant improvement of mechanical properties.

Integration of chondral phase and osseous part via stereolithography was carried out by anchoring a cured PEG hydrogel tightly to the underlying ceramic substrate [25]. Other works have investigated innovative bilayered porous silk fibroin-based scaffolds (Figure 2), developed by combining a horseradish peroxidase (HRP)-crosslinked silk fibroin (SF) layer with a HRP-crosslinked SF/ β -Tricalcium phosphate layer [26].

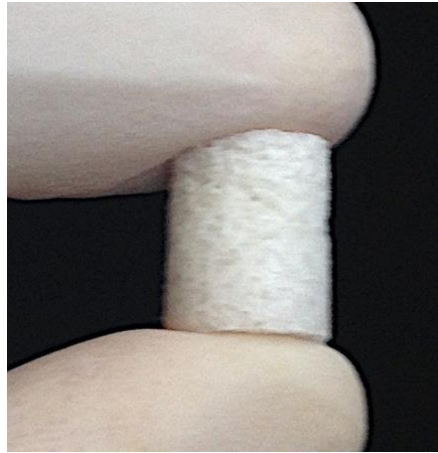


Figure 2 Bilayered porous silk fibroin-based scaffolds, combining a horseradish peroxidase (HRP)-crosslinked silk fibroin (SF) layer with a HRP-crosslinked SF/ β -Tricalcium phosphate layer. Courtesy University of Minho.

Liu C. and Blunn G.[27] have patented a biomimetic OC scaffold, by a gradient structure formed by titanium matrix, PLA junction and PLGA infiltrated collagen layer (Figure 3).

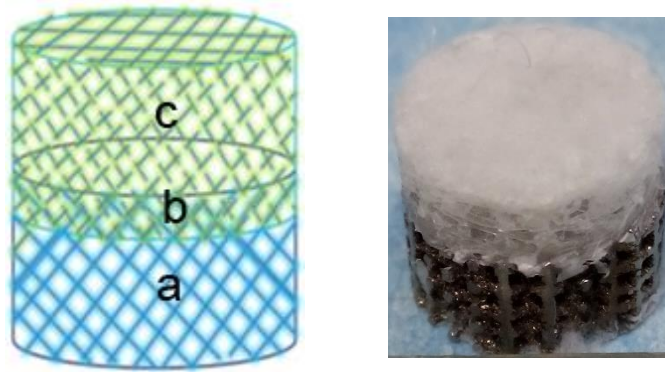


Figure 3. Gradient structure. a: Titanium matrix b: PLA junction c: PLGA infiltrated collagen layer. Courtesy University College London.

Another promising procedure is the opportunity of **Functionally Graded Materials (FGM)**, which in the context of AM is named **FGAM (functionally graded additive manufacturing)**

FGAM is a single additive manufacturing by gradationally mixing materials or modifying process parameters to fabricate freeform geometries with variable-property within one component. Functionally graded materials can be classified as follows (Figure 4):

- **Chemical composition FGM** - With two options: a) single phase as a result of the solubility of the chemical elements of one phase in the other phase. Varying chemical composition because of the solubility; b) Multiphase chemical composition. The phases and chemical composition are made to vary across the bulk volume of the material.
- **Porosity /cellular gradient FGM-** a) Porosity/cellular density gradation: The porosity density is produced with the density of porosity changing with respect to the spatial position across the volume of the material; b) Pore/cell size/shape gradation: Varying the pore/cell sizes or the pore shape, or both.
- **Microstructure gradient FGM-** The graded microstructure would result in a gradual change of the material properties with respect to position.

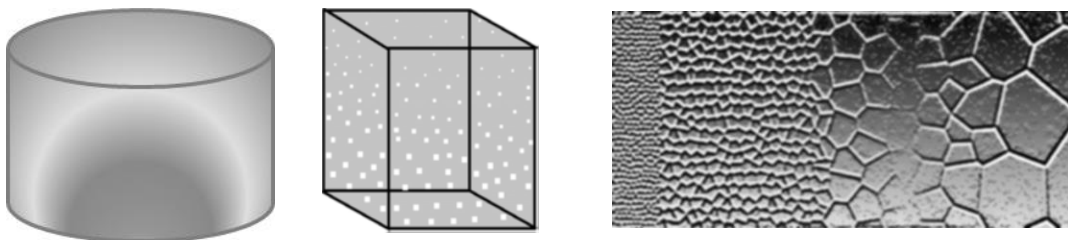


Figure 4. FGM. a. Chemical composition FGM. b. Porosity FGM. c. Microstructure FGM

Many applications of FGAM have been carried out in the medical field so far [28]. Chua et al. [29], and Sudarmadji et al. [30], presented a methodology for designing functionally graded tissue engineering scaffolds. It was composed of a library of 13 polyhedral geometric models which were obtained using Boolean operations to design an optimum scaffold. Yoo et al. [31], presented another general design framework for 3D internal scaffold architectures to match desired mechanical properties and porosity simultaneously.

1 In order to facilitate the manufacturing process, of OC scaffolds with FGM property, in a
2 bioplotter the following capabilities should be implemented:

- 3 • Capabilities for multi-material and modification of composition of each material (for
4 example with multi-feeder and mix chamber).
- 5 • CAD software with option of defining graded material in the 3D solid file.
- 6 • CAE software (FEM analysis) suitable to calculate with graded material.
- 7 • Exchange file from CAD to AM system with the option of FGAM. The well-known STL
8 file does not implement this option.

9
10
11 There is a lack of CAD/CAE systems with capabilities of FGM , so it limits the automatic process
12 from CAD to 3D printed FGAM, requiring additional tools for achieving a real FGAM.
13 Nevertheless, different initiatives are taking place such as the exchange file formats such as AMF
14 and FAV. These new formats will necessarily be the replacement of STL in the future although
15 there is still a **slow process of implementation in the commercial CAD systems**.

16
17
18 **Additive Manufacturing Format (AMF)** has been developed in the context of an ISO-ASTM
19 standard, ISO/ASTM 52915:2016 [32]. This format is very suitable for multi-material
20 specification, mixed graded materials, composites and porous materials. There are three options
21 for enabling FGAM:

- 22 • Representation of FGAM by a mathematical function. A relevant utility is the element
23 <composite> that is used to specify the ratio of the composition as a constant or an
24 equation dependent on the x, y and z coordinates.
- 25 • Volume texturing, allowing to store the distribution in space of a certain material through
26 a sequence of 2D textures, mapped in the volume of the object.
- 27 • AMF supports voxel representation, which is the three-dimensional equivalent of pixels.
28 Common uses of voxels include volumetric imaging in medicine. The advantage of this
29 is the option of assigning a particular material to one voxel.

30
31
32 Although many of the capabilities of AMF have been already included in many CAD software,
33 unfortunately some of them, suitable for FGAM, are still under development.

34
35
36 **Fabricatable voxel (FAV)**, created by Fuji Xerox [33] , expresses 3D data in the form of voxels
37 arranged three-dimensionally. For each voxel, users can define various attribute values, including
38 colour information and material information. Users can also control the relationships (e.g.,
39 connection strength) between different voxels. With this data format, it is possible to create
40 designs with multiple materials.

41 42 43 44 45 **PROPOSED METHODOLOGY TO FABRICATE FUNCTIONALLY GRADED OC** 46 **SCAFFOLDS**

47
48
49 Although there are some gaps to fully produce functionally graded OC scaffolds, due to
50 limitations in the FGAM technology as discussed in the previous section, an ideal general
51 methodology could be approached (Figure 5) to improve the existing procedures. In this
52 methodology the 3D geometry could start from 3D CAD (as usual) or from 3D image coming
53 from μ CT with voxels as basic element, mimicking, for example, a Harvesian architecture [34].
54 Mechanical analysis by Finite Elements Method (FEM) allows to predict mechanical behaviour
55 but this approach proposes also a **dynamic optimization**. The concept of this **dynamic**
56 **optimization** is to consider the modification (depending on the time) of either geometry or
57 physical properties of the material due to the degradation process of the biomaterial and the new
58 cell tissue in the scaffold. In case of FGAM OC scaffold, this dynamic optimization enables
59
60
61
62
63
64
65

optimal design and distribution of material but taking into account constraints regarding viability and efficiency of cell culture (for instance, level of porosity). Some authors have been working in optimization of lattice structures when geometry is changing with the time. For example, R. Paz et al. [35], optimized a 4D printing geometry, of shape memory part, for two different scenarios when an external stimuli deforms the part, based on genetic algorithm as method for optimization. Once the dynamic optimal solution is achieved, the 3D geometry is exported either to AMF or FAV and the slicer interface imports such an exchange format to define the routes, processing parameters and print heads, combining the graded materials to make the graded OC scaffold in a multi-head bioplotter .Note that a specific strategy is needed when combining hydrogels or biopolymers melting at very low temperature with those biopolymers at high temperature (for example programming some delays to cold the deposited biomaterial).

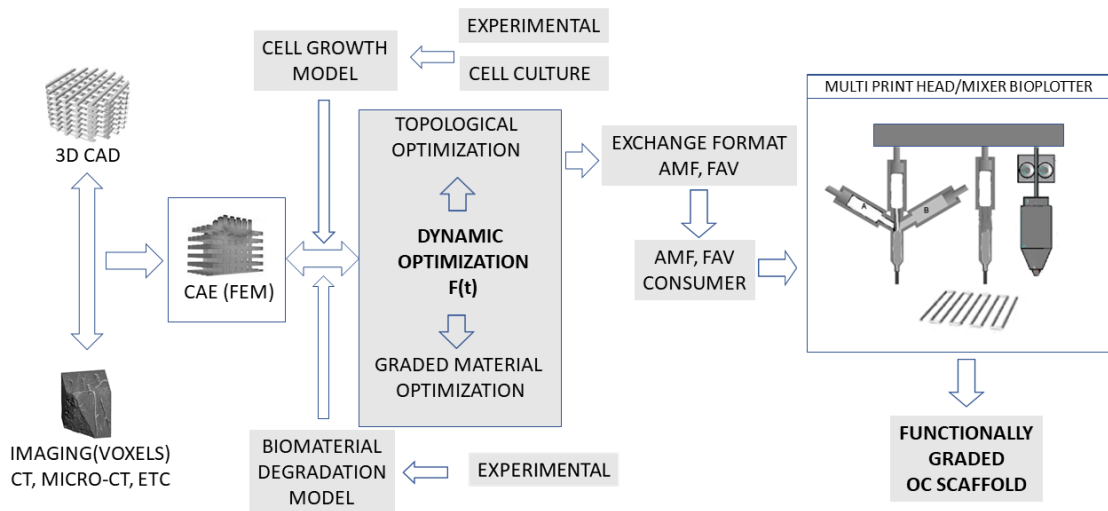


Figure 5. General methodology for design and manufacturing Functionally Graded OC scaffolds

ACKNOWLEDGEMENT

The authors would like to thank H2020-MSCA-RISE program, as this work is part of developments carried out in BAMOS project, funded from the European Union's Horizon 2020 research and innovation programme under grant agreement N° 734156

REFERENCES

1. Cucchiarini M, Girolamo L, Filardo G, Oliveira J.M. ,Orth P, Pape D, Reboul P (2016), Basic science of osteoarthritis, *Journal of Experimental Orthopaedics*, 3(1): 22. doi:10.1186/s40634-016-0060-6.
2. Canadas RF, Pina , Marques AP, Oliveira JM, Reis RL (2014), *Cartilage and Bone Regeneration – How close are we to bedside?*, *Translating Regenerative Medicine to the Clinic*, Elsevier, 89-106
3. Kon E, et al. (2011), Novel nano-composite multilayered biomaterial for osteochondral regeneration: a pilot clinical trial, *Am J Sports Med*, 39(6): 1180-90

- 1 4. Filardo G, et al (2013), Treatment of knee osteochondritis dissecans with a cell-free biomimetic
2 osteochondral scaffold: clinical and imaging evaluation at 2-year follow-up, *Am J Sports Med*,
3 41(8):1786-93
- 4 5. Bekkers JE, et al (2013), Articular cartilage evaluation after TruFit plug implantation analyzed
5 by delayed gadolinium-enhanced MRI of cartilage (dGEMRIC). *Am J Sports Med*, 41(6): 1290-
6 5
- 7 6. Verhaegen J, et al (2015), TruFit Plug for Repair of Osteochondral Defects-Where Is the
8 Evidence? Systematic Review of Literature, *Cartilage*, 6(1): 12-9
- 9 7. Irion VH, Flanigan DC (2013), New and Emerging Techniques in Cartilage Repair: Other
10 Scaffold-Based Cartilage Treatment Options, *Operative Techniques in Sports Medicine*, 21(2):
11 125-137
- 12 8. Filardo, G., et al (2013), Osteochondral scaffold reconstruction for complex knee lesions: a
13 comparative evaluation. *Knee*, 20(6): 570-6
- 14 9. Kon, E., et al (2014), A one-step treatment for chondral and osteochondral knee defects: clinical
15 results of a biomimetic scaffold implantation at 2 years of follow-up. *J Mater Sci Mater Med*,
16 25(10): 2437-44
- 17 10. Kon E, et al (2014), Tibial plateau lesions. Surface reconstruction with a biomimetic
18 osteochondral scaffold: Results at 2 years of follow-up, *Injury*, 45(6): p. S121-5
- 19 11. Christensen BB, et al (2016), Poor osteochondral repair by a biomimetic collagen scaffold: 1-
20 to 3-year clinical and radiological follow-up. *Knee Surg Sports Traumatol Arthrosc*, 24(7): 2380-
21 7
- 22 12. Kon E, et al (2016), A novel aragonite-based scaffold for osteochondral regeneration: early
23 experience on human implants and technical developments, *Injury*, 47(6): 27-32
- 24 13. Ondresik M, et al (2016), Management of knee osteoarthritis. Current status and future trends,
25 *Biotechnol Bioeng*, 114(4):717-739
- 26 14. Athanasiou KA, Darling EM, Hu JC (2009), Articular cartilage tissue engineering, *Synthesis*
27 *Lectures on Tissue Engineering*, 1(1): 1-182
- 28 15. Natoli RM, Revell CM, Athanasiou KA (2009), Chondroitinase ABC treatment results in
29 greater tensile properties of self-assembled tissue-engineered articular cartilage, *Tissue*
30 *Engineering Part A*, 15(10): 3119-3128
- 31 16. Karageorgiou V, Kaplan D (2005), Porosity of 3D biomaterial scaffolds and osteogenesis.
32 *Biomaterials*, 26(27): 5474-5491
- 33 17. Kim K, et al (2010), Stereolithographic bone scaffold design parameters: osteogenic
34 differentiation and signal expression, *Tissue Engineering Part B: Reviews*, 16(5): 523-539
- 35 18. Monzon MD, Ortega Z, Martínez A, Ortega F (2015), Standardization in additive
36 manufacturing: activities carried out by international organizations and projects, *Int J Adv Manuf*
37 *Technol* 76: 1111-1121
- 38 19. ISO/ASTM 52900:2015. Additive manufacturing — General principles — Terminology
- 39 20. Monzon M., et al (2017), Anisotropy of Photopolymer Parts Made by Digital Light
40 Processing, *Materials*, 10: 64

- 1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
21. Taniguchi N, et al (2016), Effect of pore size on bone ingrowth into porous titanium implants fabricated by additive manufacturing: An in vivo experiment, *Mater Sci Eng C*, 59:690-701
 22. Kim JD, et al (2010), Piezoelectric inkjet printing of polymers: Stem cell patterning on polymer substrates, *Polymer*, 51(10):2147-54.
 23. Hölz K, et al (2016), Bioink properties before, during and after 3D bioprinting, *Biofabrication* 8(3): 032002
 24. Shim J, et al (2011), Development of a hybrid scaffold with synthetic biomaterials and hydrogel using solid freeform fabrication technology, *Biofabrication*, 3(3): 034102
 25. Li X, et al (2015), Biomimetic biphasic scaffolds for osteochondral defect repair, *Regen Biomater*, 2(3): 221–228
 26. Viviana P. Ribeiro, Sandra Pina, João B. Costa, Ibrahim F. Cengiz, Luis García-Fernández, Mar Fernández-Gutierrez, Ana L. Oliveira, Julio San-Román, Joaquim M. Oliveira and Rui L. Reis. Novel bilayered silk fibroin-based composite scaffolds for osteochondral regeneration. Submitted
 27. Patent pending WO2017118863 A1 Chaozong LIU, Gordon Blunn
 28. Pei E, et al (2017), A study of 4D printing and functionally graded additive manufacturing, *Assembly Automation*, 37(2): 147-153
 29. Chua CK, Sudarmadji N, Leong KF (2008), Functionally graded scaffolds: the challenges in design and fabrication processes, in da Silva Bártolo, *Virtual and Rapid Manufacturing: Advanced Research in Virtual and Rapid Prototyping*, CRC Press, 115-120
 30. Sudarmadji N, et al (2011), Investigation of the mechanical properties and porosity relationships in selective laser-sintered polyhedral for functionally graded scaffolds, *Acta Biomaterialia*, 7: 530-537
 31. Yoo DJ (2013), Heterogeneous porous scaffold design using the continuous transformations of triply periodic minimal surface models, *International Journal of Precision Engineering and Manufacturing*, 14(10): 1743-1753
 32. ISO/ASTM 52915:2016. Specification for additive manufacturing file format (AMF) Version 1.2
 33. Fuji Xerox (2017) The New 3D Data Format FAV. Available at: <http://www.fujixerox.com/eng/company/technology/communication/3d/fav.html>
 34. <https://2017.biomaterials.org/sites/default/files/abstracts/0811.pdf>
 35. Paz R, et al (2017), Lightweight parametric design optimization for 4D printed parts, *Integrated Computer-Aided Engineering*, 24(3): 225-240

Table 1. Commercial bioplotters and biomaterials for 3D printing

Model, Company	Material
3D Bioplotter, Envisiontec	Ceramic/metal pastes (HA, TCP, Ti), thermoplastics (PCL, PLLA, PLGA), Hydrogels (Agar, Gelatin, Soy, Hyaluronic acid, Alginate, fibrin, chitosan, collagen), acrylates (UV curing)
BIO X., CELLINK	Alginate/nanocellulose, collagen, gelatin methacrylate, Pluronic F127 (polypropylene glycol/polyethylene glycol), TCP, PCL,
Biofactory, RegenHU	PEG, gelatin, hyaluronic acid-based, Calcium phosphate
Allevi 6, Allevi	PLGA, PCL, Pluronic 127, gelatin methacrylate, collagen, alginate, fibrin, Polyethylene glycol diacrylate

